

Telepac® Infection Protection



Fairmont Medical's single use Telepac has revolutionised telescope reprocessing, storage and transport in hospital facilities.

The Telepac is totally recyclable and carries a 7 rating. Safe disposal may also be achieved in the same way as non woven sterilisation wraps.



Telepac's clear shell helps reduce incorrect telescope selection.



Soft malleable concertina handle, allows for easy telescope ejection during aseptic handover.

Easy grip neck allows for control during hand over. It's unique shape prevents movement of tray inside Telepac.

Security Lock provides a tamper evidence. A visible locking system, for peace of mind.



-Fairmont
MEDICAL

- Telepac is a single use product, which requires no cleaning.
- Complies with AS/NZS 4187:2014 for rigid telescopes.
- 12 Telepac's fit comfortably into a STERRAD® low temperature gas plasma sterilizer.

- Reduces wrapping time.
- Reduces sterilising cycle costs.
- Reduces the risk of perforation.
- Telepac provides safe transportation.
- Saves on cleaning time and materials.
- Easy identification.


Telepac is available for both:



Autoclave -
High-pressure saturated steam at 134 °C



Low Temperature Sterilisation -
Hydrogen peroxide gas plasma

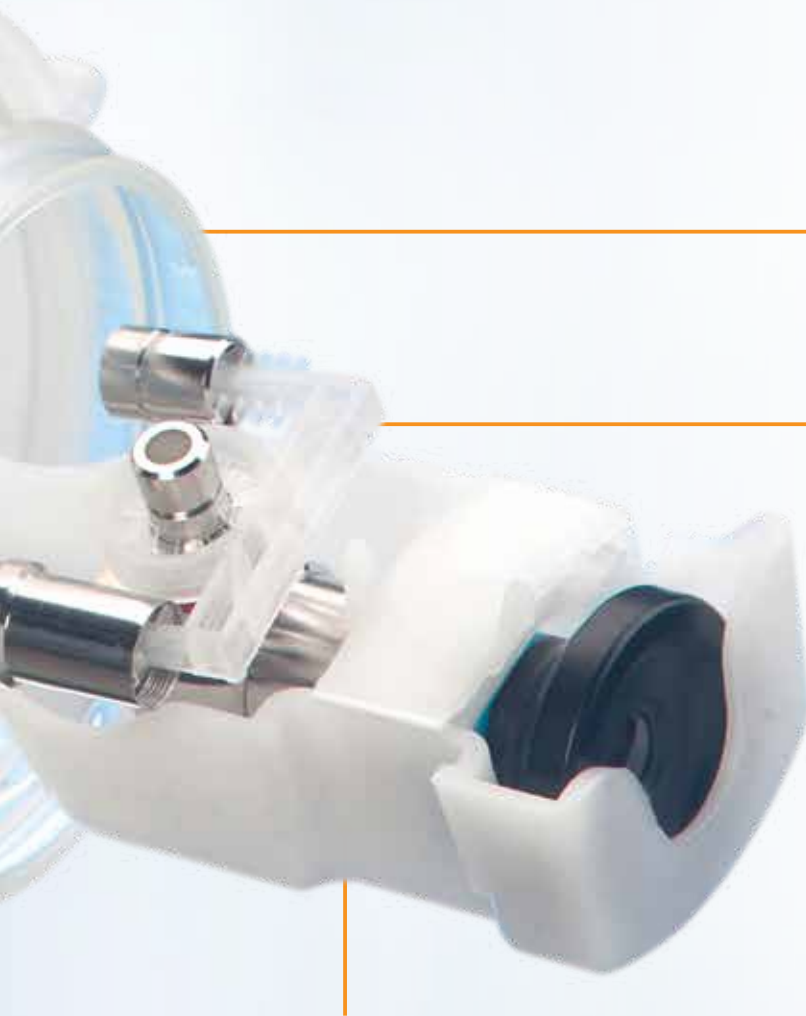

Telepac's clear shell helps reduce incorrect telescope selection.

Light Post Adaptor Mount allows integrated storage of telescope light post adaptors.

Colour coded lid system allows telescopes to be quickly and easily identified. Lid flat section enables Telepac to be clearly labelled for traceability and sterilisation.



Telepac offers the choice of a disposable or reusable tray. Inner tray protects scopes in theatre whilst on stand, providing greater protection from damage if accidentally dropped.



Telepac® Hospital Cycle

Sterilisation Department

4. Sterilising

Telepac is validated for all sterilising methods, including steam and low temperature. 12 Telepac's fit comfortably into a STERRAD® low temperature gas plasma sterilizer. Designed with a non woven built in barrier, it allows for penetration and removal of sterilising gases and steam. Low temperature sterilisation cycles are commonly subjected to cycle failures due to the presence of moisture residue (wetpacks). Telepac avoids this from occurring.

3. Apply Tamper Evidence Seal

Screw lid on to align tamper evidence seal. Attach tamper evidence lock through two eyelets on lid. Tamper evidence breaks when lid is opened. Colour coded lids can be clearly labeled for traceability and sterilisation processes.

2. Loading Telepac

Load inner tray and telescope inside Telepac. Telepac provides safe transportation.

1. Preparing Telepac

Load washed telescope into inner tray and clip into place.

Load light post adaptor mount and clip to telescope.



Optional reusable stainless steel telescope trays available. Ideal for washer disinfectors.




Scan the QR
code to view
the Telepac®
process

Operating Theatre

5. Storage

Telepac's modular racking system provides a safe and efficient storage facility. Colour coded system allows telescopes to be quickly and easily identified.

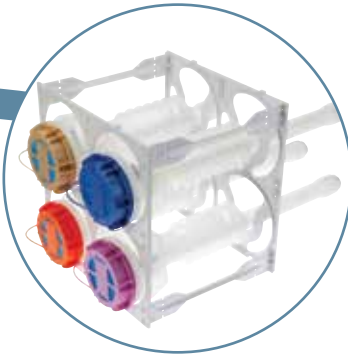

6. Hand Over

Twist lid to release tamper evident lock. Simply push concertina handle and the telescope is ejected ready for hand over to scrub nurse.



7. Telescope Usage

The unique Telepac design provides a safe and easy aseptic presentation of telescope in theatre. Inner tray protects scopes, providing greater protection if accidentally dropped.




8. Return to CSSD

Used telescope is replaced in inner tray and re-inserted into Telepac prior to return to CSSD.

Telepac protects telescope from damage during transportation to and from theatre.



Telepac® Storage

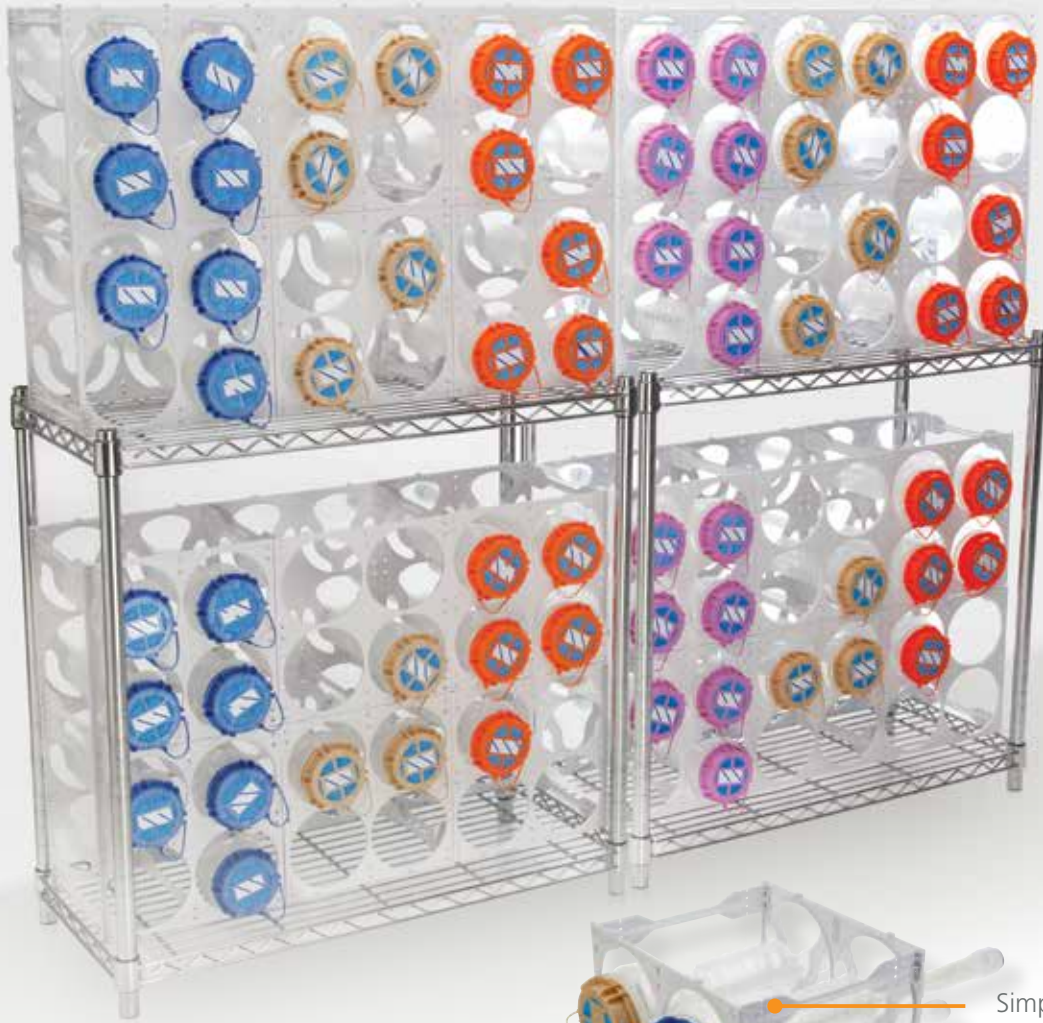


Telepac's lightweight modular racking system provides a safe and efficient storage facility and is supplied free of charge.

Simple cliplock construction

Telepac® Decontamination Tray

- Perforated reusable 316 stainless steel tray
- Designed for use in various instrument washers and disinfectors
- Tray enables direct transfer of telescope to Telepac for processing
- Outer Dimensions:
L480 x W250 x H50 mm

Adjustable silicone telescope tray holders provide secure telescope tray attachment

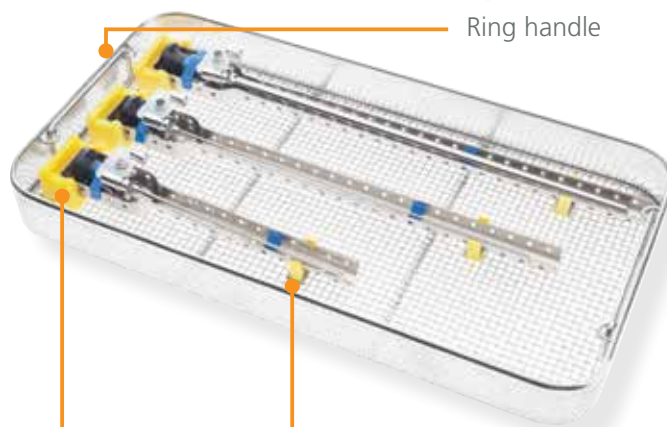

Ring handle



Fairmont
MEDICAL

Telepac® Specifications


Autoclave Compatible - Non-Sterile, Disposable

Product	Product Code With Tray	Product Code Without Tray	Description	Colour Lid	Telescope Compatible	Box Qty
	DTP6005	DTP6105	Small Body	Gold	Suits 2.7mm and 4mm. Arthroscopes / ENT to a maximum working length of 187mm	30
	DTP6010	DTP6110	Large Body	Pink	Suits 4mm Uro/Gyn scopes with a working length of 312-336mm	24
	DTP6020	DTP6120	Large Body	Blue	Suits 5, 6.5 and 10mm. Laparoscopes with a working length of 312-336mm	24
	DTP6040	DTP6140	Extra Large Body	Orange	Suits 10mm. Laparoscopes with a working length of 344mm	24


Low Temperature Compatible - Non-Sterile, Disposable

Product	Product Code With Tray	Product Code Without Tray	Description	Colour Lid	Telescope Compatible	Box Qty
	DTP7005	DTP7105	Small Body	Gold	Suits 2.7mm and 4mm. Arthroscopes / ENT to a maximum working length of 187mm	30
	DTP7010	DTP7110	Large Body	Pink	Suits 4mm Uro/Gyn scopes with a working length of 312-336mm	24
	DTP7020	DTP7120	Large Body	Blue	Suits 5, 6.5 and 10mm. Laparoscopes with a working length of 312-336mm	24
	DTP7040	DTP7140	Extra Large Body	Orange	Suits 10mm. Laparoscopes with a working length of 344mm	24

Telescope Tray Stainless Steel - Non-Sterile, Reusable

Product	Product Code	Description	Telepac Compatible Model	Box Qty
	TPT5100	Telescope Tray Stainless Steel - Small	DTP6005, DTP7005	Each
	TPT5200	Telescope Tray Stainless Steel - Large	DTP6010, DTP6020, DTP7010 & DTP7020	Each
	TPT5300	Telescope Tray Stainless Steel - X-Large	DTP6040 & DTP7040	Each

Telepac Storage Rack - Non-Sterile

Product	Product Code	Box Qty
	TPRACK1	Each

Telepac Decontamination Tray - Non-Sterile

Product	Product Code	Box Qty
	TDT8000*	Each
* Note. Telescopes not included		



Corporate Office
Fairmont Medical
11 Scoresby Road Bayswater 3153 VIC
Ph 1300 972 088
Ph International +613 9720 8840
Fx International +613 9237 9399

UK Head Office
Fairmont Medical Products Ltd
Elizabeth House
28 Baddow Road Chelmsford
Essex CM2 0DG
Ph: +44 (0)1245 206800

